Print on plain white paper (both sides) - Part # 122919

INSTRUCTIONS
INSTALLATION AND OPERATING

for the Unit Mounted Ultrasonic Scaler System

PART I - INSTALLATION

1. Mount the scaler system inside the console by attaching it to the inside and bottom covers using the velcro strips provided (See Figure 1).
2. Make the tubing connections as shown, matching the tags (A,B,C) and colors (See Figure 2).
3. Attach the connector to the corresponding connector from the unit.
4. Plug the power cord into the outlet provided inside the console.

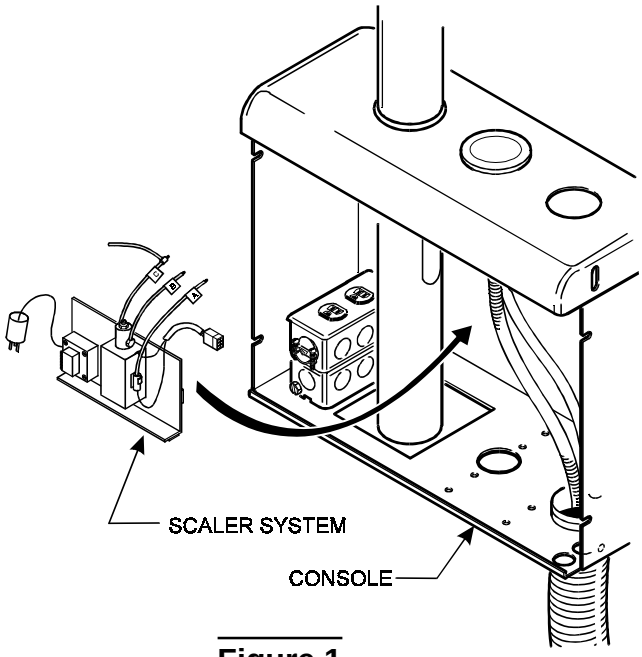

Figure 1

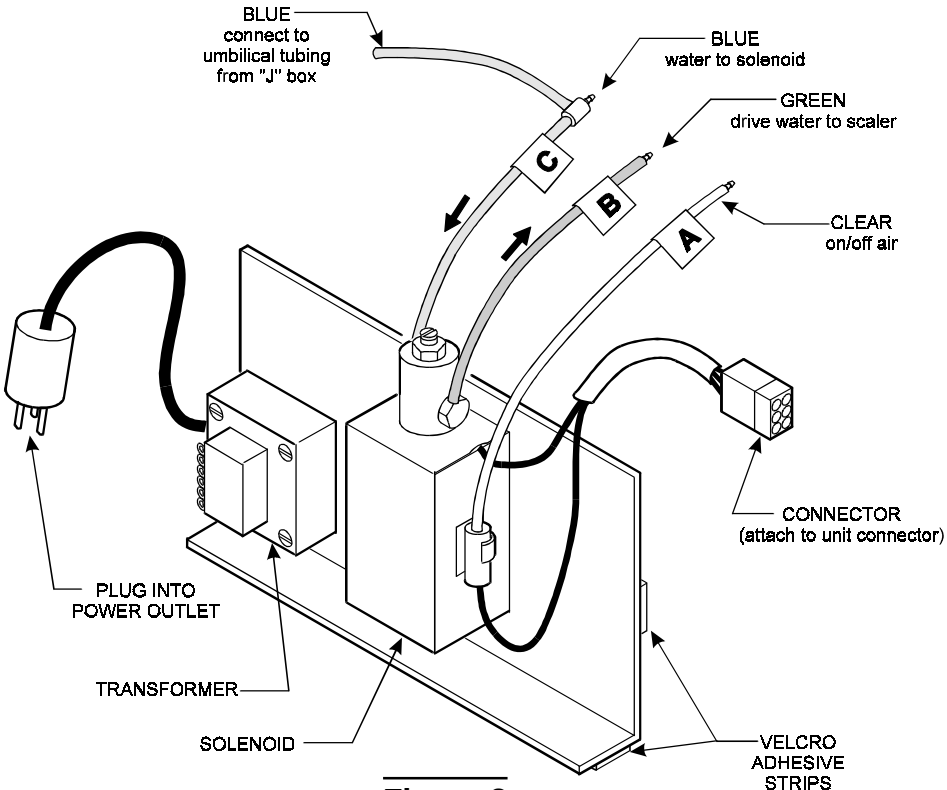

Figure 2

PART II - OPERATION

1. Push the ultrasonic insert into the handpiece with a gentle push-twist motion. Do not force into place (See Figure 3).
2. Lift the handpiece from its holder and depress the foot controller. This will cause the handpiece to operate.
3. Adjust the intensity using the intensity control knob on the unit head (See Figure 4).
4. The water volume may be adjusted by the water volume control knob. This control is located on the front of International units or under the lift-off cover on Asepsis 21 units.



Figure 3

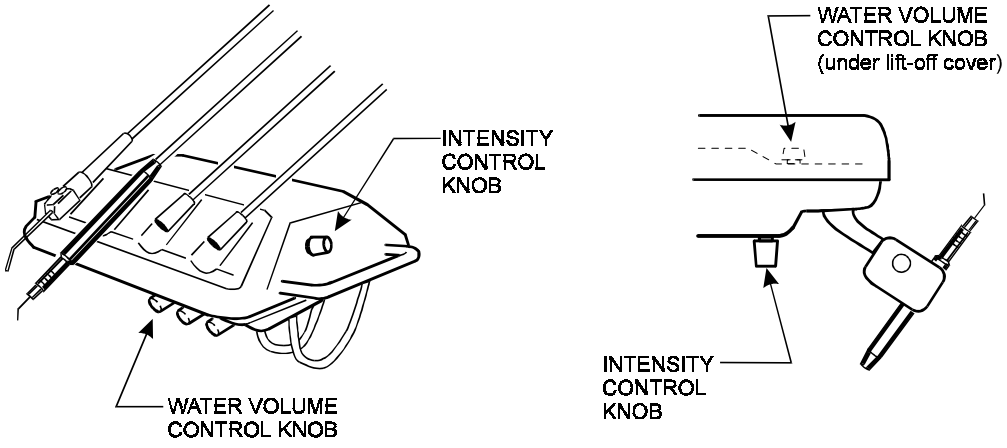

Figure 4

Knight®
by Midmark
Midmark Corporation • P O Box 286 • 60 Vista Drive
Versailles • Ohio • 45380-0286 • www.midmark.com
Phone: 937-526-3662 Fax: 937-526-5542